


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

MAY 23 2011

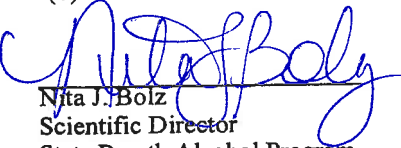
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program


Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130302
Name		CHRIS HILL	ID# 3839 Date 5/19/11
A	Agency	AST	Phone # 486-4121
Instrument Location KODIAK POST INTERVIEW ROOM			
Alco S/N		X124658	Target Value .084 High Pressure 1140
B	Alco Test Value Average		.086 .086
	1 st Alco		2 nd Alco
Signature 			
(OVER)			


(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 15 day of JUNE, 2010. 


(Notary Seal Stamp)
Daniel L. Nicholas Kyle KLOPPER
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130302

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130302

MAY 19, 2011

OPERATOR'S NAME:

HILL C W

OPERATOR'S NUMBER: 3829

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/NI :

X

O.L. #: X

DEPT/AGENCY: KODU

CASE/REPORT: 0

TEST TYPE: V

ALCO TARGET VALUE: .004

ALCO S/N: X124658

--- BREATH ANALYSIS ---

.004 ADJUSTED FOR 29.75 in

ALCO TARGET .003 10:23

BLANK TEST .000 10:24

INTERNAL STANDARD VERIFIED 10:24

ALCO TV 29.75 in .006 10:24

BLANK TEST .000 10:25

SUBJECT SAMPLE .000 10:26

BLANK TEST .000 10:26

ALCO TV 29.75 in .006 10:27

BLANK TEST .000 10:27

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130302

MAY 19, 2011

TIME 10:28

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 01/05/09

HEATERS

SAMPLE CHAMBER: 1.0

BREATH TUBE: 4.0

BAROMETER: 29.75 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!""&%'()*+,-./0123456789:;<=>?@ABCDEF6
HIJKLMNOPQRSTUVWXYZ[\]^_`ab cde fgh i j k l m n o
p q r s t u v w x y z { | } ~